




**Lab ID** TM0585  
**Scheme** Therapeutic Drugs (TDM)  
**Analyte** Trazodone  
**Round** 160  
**Issued** 03 March 2017

**Results**

Sample	Method	Result	Unit	z/z' score
PS29	LCMS & MS/MS	670.00	µg/L	1.22

**Data Statistics**

Sample	PS29
No. Results	22
No. Excluded Results	0
Mean	547.93 µg/L
Median	557.15 µg/L
Standard Deviation	91.494 µg/L
Robust Standard Deviation	92.688 µg/L
Result Range	253.88 to 670.00 µg/L

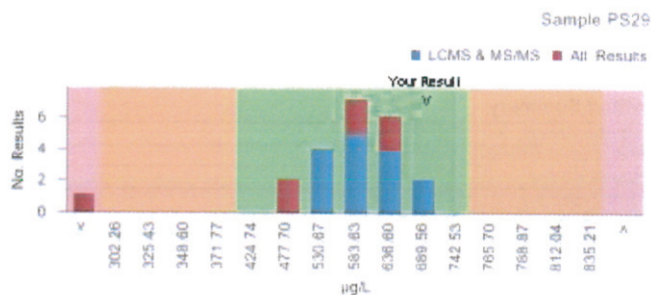

Note: The concentration value (x-axis) is the upper limit of a range of values.

**Performance Statistics**


Sample	PS29
Assigned Value	557.15 µg/L
Uncertainty of Assigned Value	24.70 µg/L
SDPA	92.688 µg/L
Spike Value	545.42 µg/L
Satisfactory Range	371.77 to 742.53 µg/L
Satisfactory z/z' scores	95.5%
Questionable z/z' scores	0.0%
Unsatisfactory z/z' scores	4.5%

**Last 9 Performance Scores**

Sample PS29 - Round	136	139	142	145	148	151	154	157	160
LCMS & MS/MS									1.22

< or > = Less/Greater than result returned, no assessment given. ZS = Zero Spiked Sample, no assessment given. Blank = No result submitted

Performance Score by Round



Performance Score by Concentration

